

Attention!

Please read this document

before unpacking your

HunterLab® Agera® L2

A60-1021-867, ver 1.0

The world's true measure of color

HunterLab

1. Unpack Your Box

Place the Agera L2 on the bench. Retain the packaging for return of the instrument to HunterLab if needed.

2. Review Your Order

Please review your order. Compare your purchase order with the shipping document from HunterLab.
If there are any discrepancies, please contact the HunterLab Customer Experience Team.


3. Select a Space for the Agera L2


The HunterLab Agera L2 Spectrophotometer is a high-precision laboratory instrument. Laboratory-grade environments are required and should be maintained to ensure precise and accurate measurements.
The table below shows instrument size and weight along with requirements for electrical and temperature/humidity.

Height	28 cm; 11.0 in
Width	21.6 cm; 8.75 in
Depth	31 cm; 12.25 in
Weight	7.7 kg; 17.0lb
Power Outlet	110-240AC
Electrical	47-63Hz Single Phase
Temperature	10° to 40° C (50° to 104° F)
Humidity	10 % to 90 % RH, noncondensing

4. Site Conditions

- Allow 20cm (8in) of unobstructed clearance on each side of the instrument.
- The instrument should be placed to **avoid *direct* sunlight** and away from windows.
- The atmosphere around the Agera L2 should be **free from *alkalis* and *acid vapors,* and *organic solvents.***
- Do not operate the Agera L2 in the presence of ***strong electrical fields***.
- ***Avoid strong vibrations* or *shocks.***
- Ensure that there are no ***heat- generating sources*** near the Agera L2.

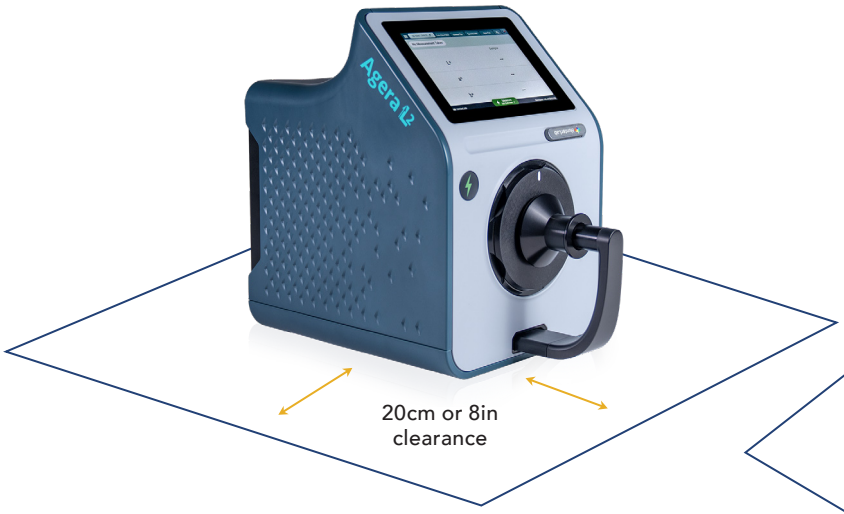

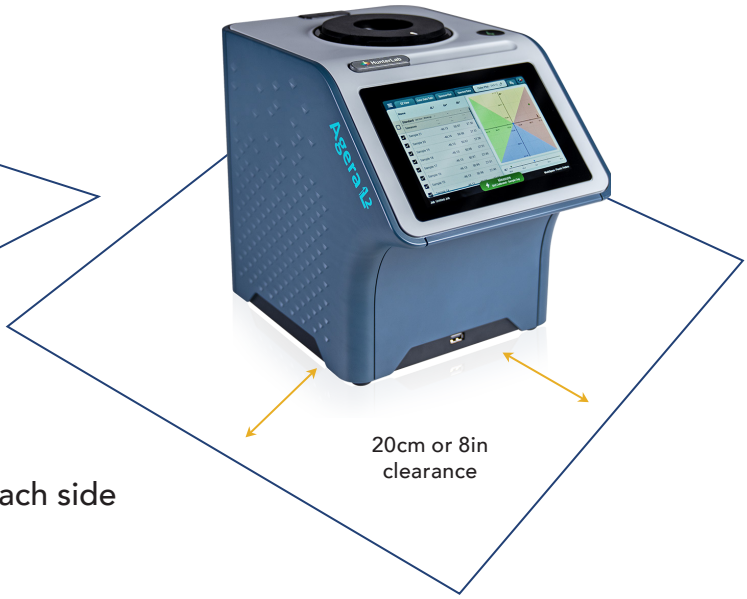

Allow 20cm (8in) of unobstructed clearance on each side of the instrument.

Note: Failure to comply with these conditions and protocols set forth in this document may adversely affect the instrument performance.



5. Safety Requirements

- UV Radiation – Wear UV protecting eye wear when viewing or observing the LEDs inside the instrument.

6. Instruction Manual


The HunterLab Instruction Manual for Agera L2 compliments the information presented here and supplies a more detailed view of operation, troubleshooting and optimization. By referring to the instruction manual, you will gain understanding of practical applications that will help you achieve excellence in using your HunterLab Agera L2 spectrophotometer.

7. Service

- Only HunterLab authorized, factory-trained representatives are permitted to service HunterLab's products.
- Do not remove any of the covers. Service is to be performed by a HunterLab service representative.

Contact the HunterLab Customer Experience Team at support@hunterlab.com if service is needed.

SCAN ME



The world's true measure of color

HunterLab

11491 Sunset Hills Road
Reston, VA 20190-5280
www.hunterlab.com