

# Attention!

## Please read this document

## before unpacking your

## HunterLab® Vista® L2

A60-1021-905, ver. 1.0

The world's true measure of color

HunterLab

## 1. Unpack Your Box

Place the Vista L2 on the bench. Retain the packaging for return of the instrument to HunterLab if needed.

## 2. Review Your Order

Please review your order. Compare your purchase order with the shipping document from HunterLab.
If there are any discrepancies, please contact the HunterLab Customer Experience Team.

## 3. Select a Space for the Vista L2

The HunterLab Vista L2 Spectrophotometer is a high-precision laboratory instrument. Laboratory-grade environments are required and should be maintained to ensure precise and accurate measurements.

The table below shows instrument size and weight along with requirements for electrical and temperature/humidity.

| | |
|---|---|
| **Height** | 17.8 cm; 7.0 in |
| **Width** | 48.6 cm; 19.1 in |
| **Depth** | 22.9 cm; 9.0 in |
| **Weight** | 6.35kg; 14.0lb |
| **Power Outlet** | 110-240AC |
| **Electrical** | 47-63Hz Single Phase |
| **Temperature** | 10 - 40°C (50 - 104°F) |
| **Relative Humidity** | 10% to 90% non-condensing |

## 4. Site Conditions

- Allow 20cm (8in) of unobstructed clearance on each side of the instrument.
- The instrument should be placed to **avoid *direct* sunlight** and away from windows.
- The atmosphere around the Vista L2 should be **free from *alkalis* and *acid vapors*, and *organic solvents***.
- Do not operate the Vista L2 in the presence of ***strong electrical fields***.
- **Avoid *strong vibrations* or *shocks***.
- Ensure that there are no ***heat- generating sources*** near the Vista L2.

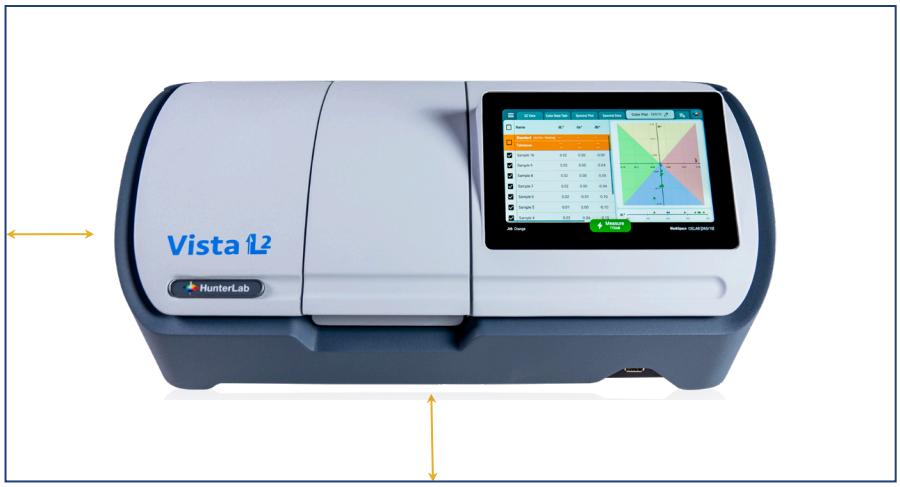


Allow 20cm (8in) of unobstructed clearance on each side of the instrument.

***Note: Failure to comply with these conditions and protocols set forth in this document may adversely affect the instrument performance.***




## 5. Safety Requirements

- UV Radiation – Wear UV protecting eye wear when viewing or observing the LED's inside the instrument.

## 6. Instruction Manual

The HunterLab Instruction Manual for Vista L2 compliments the information presented here and supplies a more detailed view of operation, troubleshooting and optimization. By referring to the instruction manual, you will gain understanding of practical applications that will help you achieve excellence in using your HunterLab Vista L2 spectrophotometer.

## 7. Service

- Only HunterLab authorized, factory-trained representatives are permitted to service HunterLab's products.
- Do not remove any of the covers. Service is to be performed by a HunterLab service representative.

**Contact the HunterLab Customer Experience Team at support@hunterlab.com if service is needed.**

SCAN ME



The world's true measure of color

HunterLab

11491 Sunset Hills Road
Reston, VA 20190-5280
www.hunterlab.com